
QUICK OPERATION GUIDE


SINGLE CHANNEL ELECTRONIC PIPETTE
PA-10 / 20 / 200 / 1200 / 10000

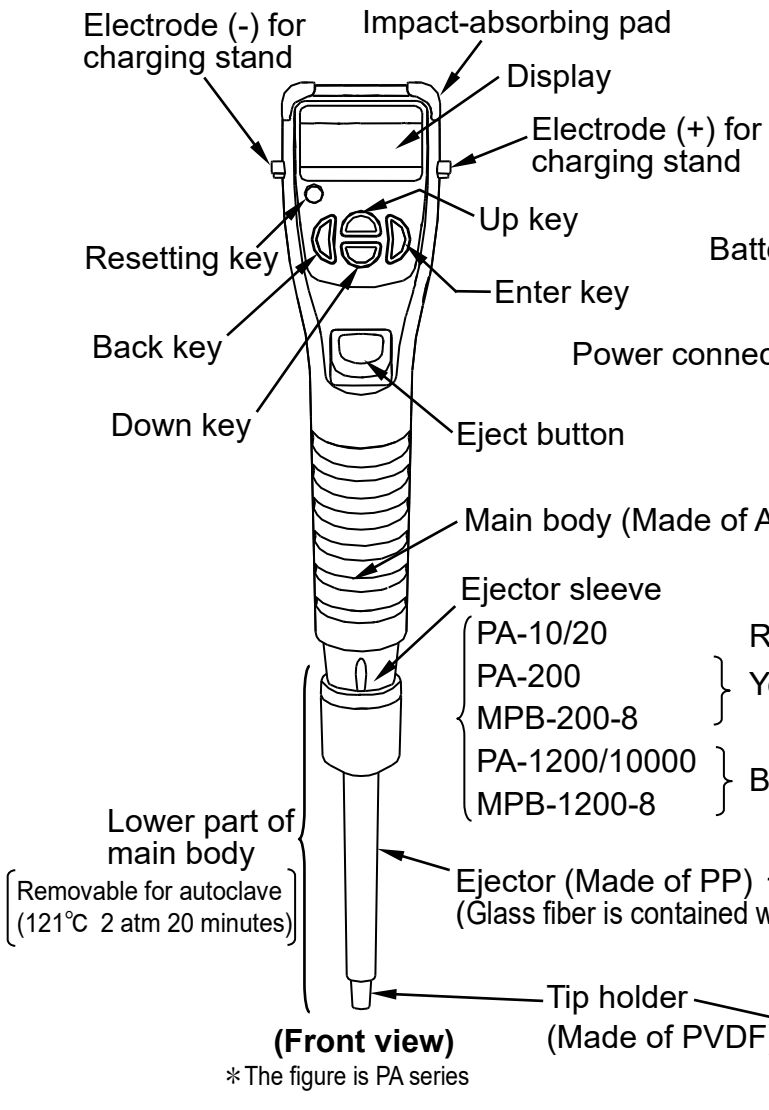

(Front view)


＊The figure is PA series

MULTI CHANNEL ELECTRONIC PIPETTE
MPB-200-8 / 1200-8

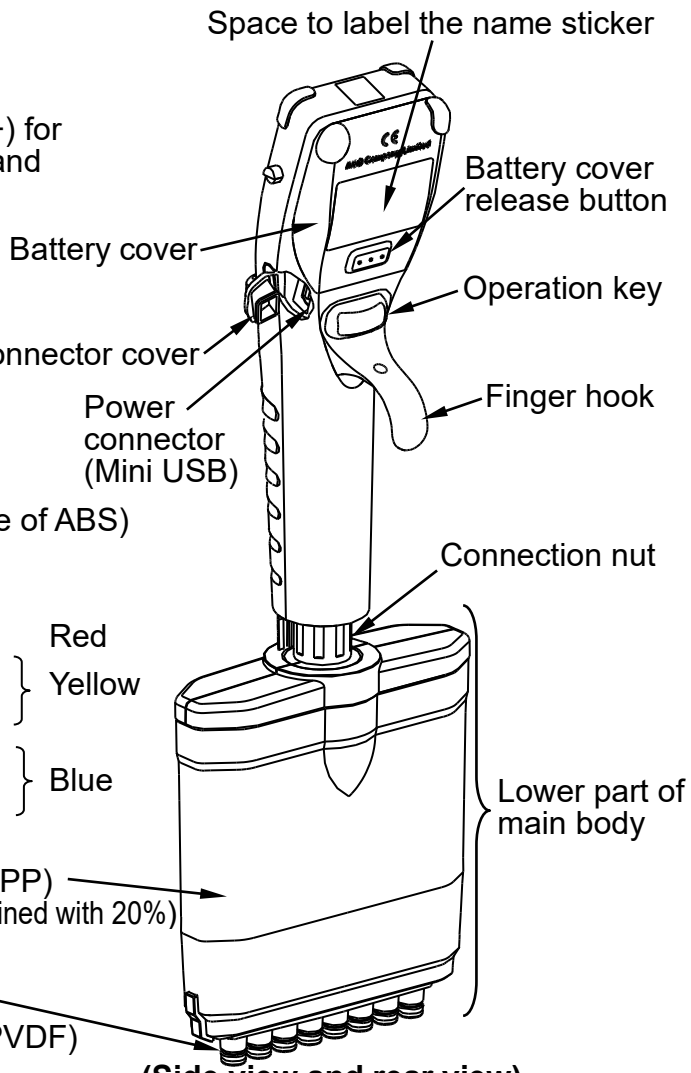

(Side view and rear view)

＊The figure is MPB series

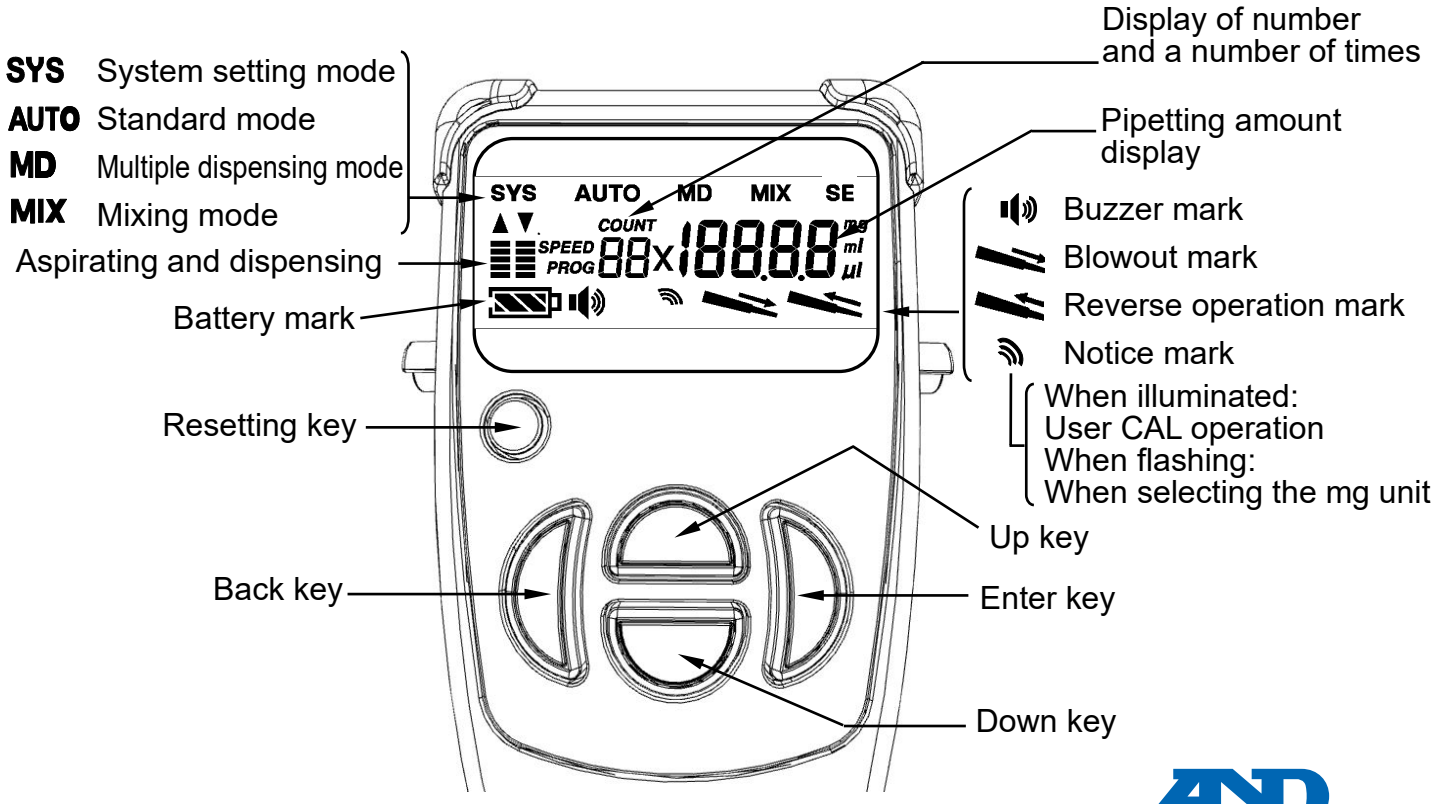


A&D Company, Ltd.

Example of the function and operation

(The following example is when using PA-200.)


Standard mode (AUTO)

Example: When dispensing with the dispensing volume of 100µL

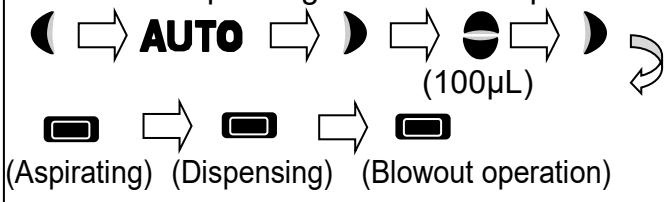


Multiple dispensing mode (MD)

Example: When multiple dispensing of 40µL ×3 times = 120µL

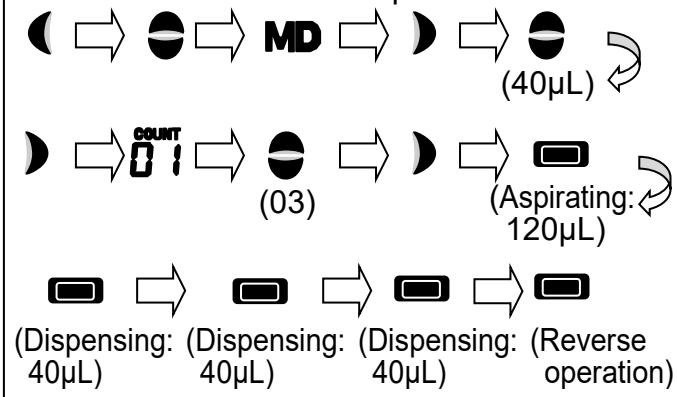


Mixing mode (MIX)

Example: When mixing with 100µL five times

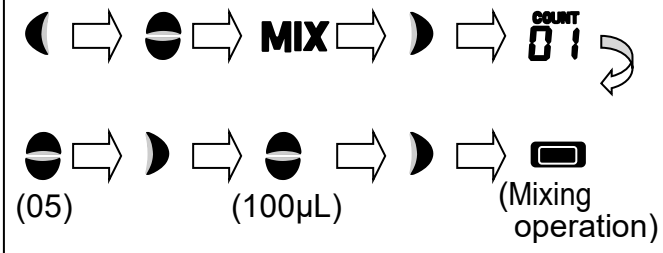


System setting mode (SYS)

Example: When setting the buzzer to OFF

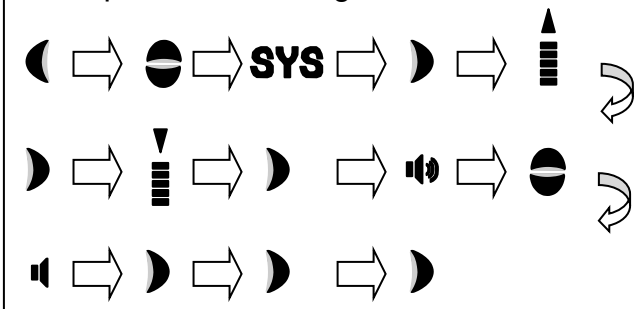


Volume adjustment function (µL adjustment function)

Example: When adjusting the dispensing amount to 190µL

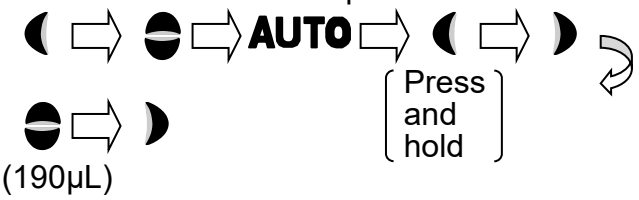


Initializing the volume adjustment

Example: When initializing the dispensing amount adjusted

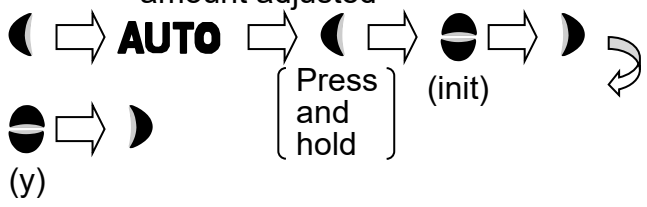


Dispensing in a unit of weight (in mg unit)

Example: When changing the unit of the dispensing amount to a unit of weight

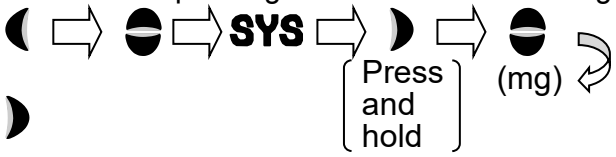

Weight adjustment function (mg adjustment function)

Example: When adjusting the dispensing amount to 190mg

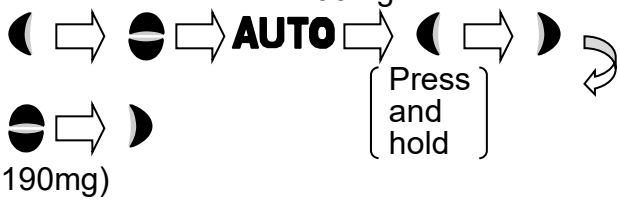

Additional contents

In operating procedure on this page, ◖ means Back key, ◓ means UP/Down key, ◗ means Enter key and ▭ means Operation key. Press these keys when operating.

Scan the code to access the instruction manual.